


NOTES: UNLESS OTHERWISE SPECIFIED

1. CONSTRUCTION:  
CONTACT SPRING: NICKEL PLATED BERYLLIUM COPPER  
INSULATOR: POLYPROPYLENE  
FRAME: NICKEL PLATED BRASS.
2. RATINGS:  
VOLTAGE: 1000V CAT II/ 1000V CAT III/600V CAT IV  
MAXIMUM CURRENT: 36 AMPS

REVISIONS			
LTR	DESCRIPTION	DATE	APPROVED

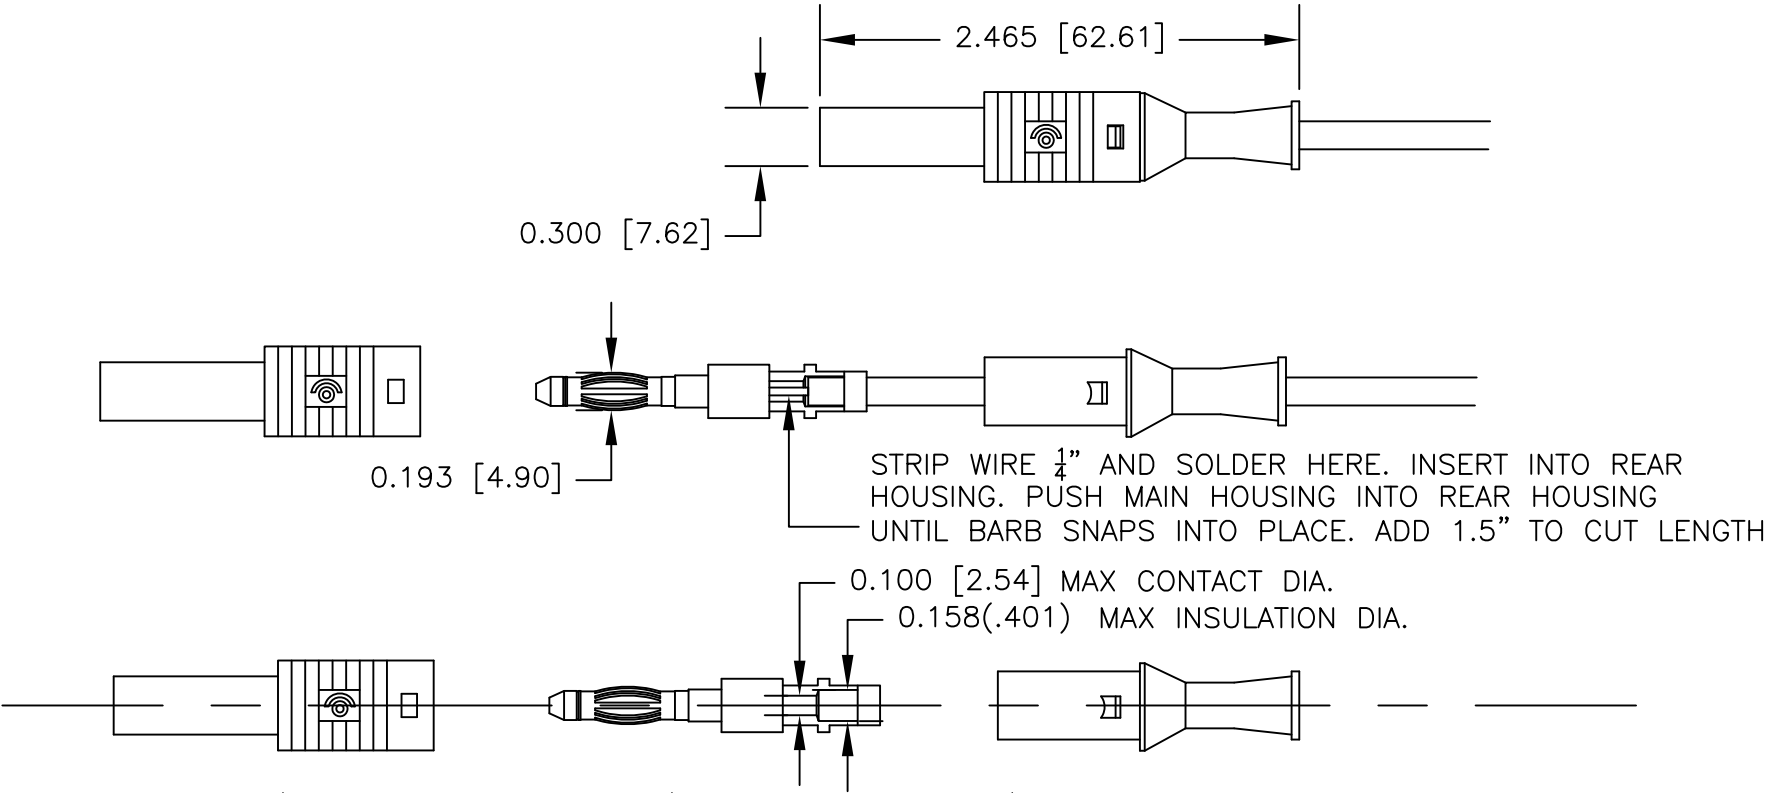

		UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ARE: FRACTIONS DECIMALS ANGLES ± .XX ± ± .XXX ±	CONTRACT NO.		<div>E-Z-HOOK®</div> <div>DIVISION OF TEKTEST INC.</div> <div>ARCADIA, CA 91006 U.S.A.</div>				
			APPROVALS	DATE	DESCRIPTION STRAIGHT SHROUDED BANANA PLUG				
			DRAWN R.L.	4/11					
		MATERIAL SEE NOTE.	APPROVED BY		SIZE CODE IDENT NO. DRAWING NO. REV. A 08505 9386				
		FINISH SEE NOTE.			SCALE 1:1 SHEET 1 OF 1				
NEXT ASSY	USED ON								
APPLICATION		DO NOT SCALE DRAWING							